





1<sup>st</sup> in India

DISINFECT  
UP TO  
99.9%

## GUARD-AIR

GERMICIDAL UNIT AND RELIABLE DRAWER - AIR PURIFIER

PATENT  
PENDING

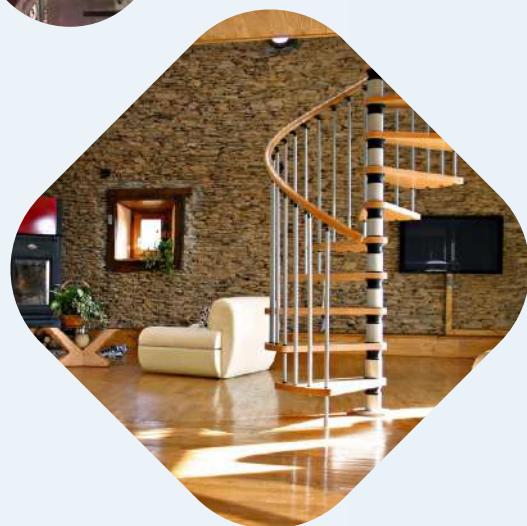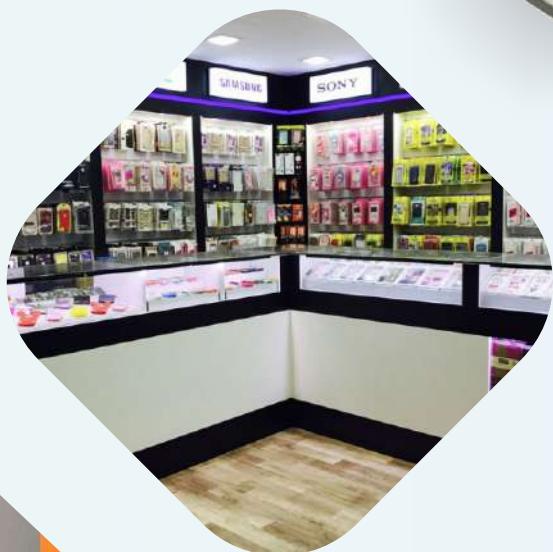

# GUARD-AIR

GUARD-AIR SPECIALLY INVENTED FOR MAKING LIFE SAFE AND PROTECTED AGAINST ALL KIND OF MICROBES. BEHIND THIS INNOVATION HUGE MARKET STUDY AND TECHNICAL EXPERTISE DONE BY SPECIAL TECHNICAL TEAM AND AFTER VERY LONG EXPERIMENTS AND LABORATORY TEST GUARD-AIR DEVELOPED. BEHIND OUR ALL INNOVATIONS THERE ARE SO MANY DOCTOR'S SUGGESTIONS AND GUIDANCE PRESENCE. GUARD-AIR IS REALLY HELPFUL FOR KEEPING SAFE FOR YOUR DAILY LIFE BELONGINGS ITEMS AND BY USING AIR PURIFIER OPTION YOU CAN ALSO MAKE YOUR SURROUNDING ATMOSPHERE SAFER FROM ALL BACTERIA VIRUS IN PRESENT AND FUTURE AS WELL. ADVANCE TECHNOLOGY INSIDE FOR AUTHENTIC LONG LASTING RESULT. PATTERN PRODUCT FOR KEEPING ALL TOGETHER.



AIR PURIFIER WORK WITH ADVANCE TECHNOLOGY WHICH KILL ALL BACTERIA AND VIRUSES PASS THROUGH DRAWER AND CHARGE AIR PARTICLE TO KILL GERMS ON ATMOSPHERE



DISINFECTION IS NOW EASY AND HASSLE FREE JUST PUT IN DRAWER AND CLOSE DRAWER PROCESS WILL AUTOMATICALLY START FOR 2MINUTES



#### PROTECTION

Use of VIGOROUS ANTIMICROBIAL SYSTEM with wavelength ensures disinfection up to 99.9%, killing bacteria & viruses on surface of any object.



#### SAFETY

Auto cut off on drawer opening ensuring complete user Safety .



#### DISINFECTION

Thoughtful placement of LED ensure all way exposure on the object placed for Disinfecting.



#### COMPACT DESIGN

Compact, contemporary & aesthetical design enhances overall ambiance of any space.

#### ADVANTAGES



CHEMICAL FREE



LEAD FREE



OZONE FREE



MERCURY FREE



ECO FRIENDLY



MAINTENANCE FREE



FAST & EASY



AIRPODS



MOBILE



GOGGLES



WALLETS



KEY



CURRENCY

DISINFECT  
ALL FREQUENTLY TOUCHED PERSONAL BELONGINGS & OBJECTS



## VIGOROUS PRODUCT PRIVATE LIMITED

AHMEDABAD, GUJARAT, INDIA

CONTACT US : (+91) 99139 53333

WEB : [WWW.VIGOROUSPRODUCT.COM](http://WWW.VIGOROUSPRODUCT.COM)



**LABORATORY REPORT**


Case ID : 011151161

Name	:GUARD -AIR (GERMICIDAL UNIT AND RELIABLE DRAWER- AIR PURIFIER) BATCH CODE :112020 - A0003 MFG : NOVEMBER 2020(EC 3 :2 MIN)	Sex/Age	: Unkown/	
Ref By	:DR KKS SIR MICRO	Dis.Loc.	:	Pt ID :
Bill. Loc.	:Supratech billing			Pt. Loc. :
Registration Date & Time	: 25-Nov-2020 20:40	Sample Type	: Plate	Ph # :
Sample Date & Time	:	Sample Coll. By	:	Ref Id :
Report Date & Time	: 01-Dec-2020 22:10	Acc. Remarks	:	Ref Id 2 :

**CORONA DISINFECTION INSTRUMENT SURVEILLANCE**
**GUARD-Air (Germicidal Unit And Reliable Drawer – Air Purifier)**
**Batch Code: 112020-A0003**
**MFG: November 2020**

**SUPRATECH MICROPATH LABORATORY & RESEARCH INSTITUTE PVT. LTD.**

Standard Organism Exposed	Vigorous Antimicrobial Light Exposure Timing	Observation	Result
Escherichia coli (ATCC 25922)	2 Minutes	No growth after 02 Minutes	Satisfactory

# For test performed on specimens received or collected from non-STMPL locations, it is presumed that the specimen belongs to the patient named or identified as labeled on the container/test request and such verification has been carried out at the point generation of the said specimen by the sender. STMPL will be responsible Only for the analytical part of test carried out. All other responsibility will be of referring Laboratory.

Approved On : Page 1 of 2

Dr. Krutarth Shah

M.D.

Microbiologist

Dr. Sandip Shah

M.D. (Path. &amp; Bact.)

Consultant Pathologist

Supratech Micropath Laboratory &amp; Research Institute Pvt. Ltd.



COLLEGE OF AMERICAN PATHOLOGISTS

## LABORATORY REPORT



Case ID : 011151161

Name	:GUARD -AIR (GERMICIDAL UNIT AND RELIABLE DRAWER- AIR PURIFIER) BATCH CODE :112020 - A0003 MFG : NOVEMBER 2020(EC 3 :2 MIN)	Sex/Age	: Unkown/	Pt ID	:
Ref By	:DR KKS SIR MICRO	Dis.Loc.	:	Pt. Loc.	:
Bill. Loc.	:Supratech billing			Ph #	:
Registration Date & Time	: 25-Nov-2020 20:40	Sample Type	: Plate	Ref Id	:
Sample Date & Time	:	Sample Coll. By	:	Ref Id 2	:
Report Date & Time	: 01-Dec-2020 22:10	Acc. Remarks	:		

**Method:** Standard ATCC strain of E.coli (Live culture) was kept in the box. Then Instrument was kept in Air purifier mode. SCDA (Soyabein casein Digest agar) plate was kept at 1 feet distance to the air outlet site. Instrument was run on Air purifier mode for 2 minutes during which contaminated air was passed through the instrument with Vigorous Antimicrobial Light ON. After 2 minutes of air exposure to the SCDA plate, it was kept in the incubator for 48 hours to check for any growth.

**Result:** No growth of Organisms after 02 Minutes of Air Exposure to Vigorous Antimicrobial Light. (Satisfactory)



TM

**VIGOROUS**  
PRODUCT PVT LTD

----- End Of Report -----

# For test performed on specimens received or collected from non-STMPL locations, it is presumed that the specimen belongs to the patient named or identified as labeled on the container/test request and such verification has been carried out at the point generation of the said specimen by the sender.  
STMPL will be responsible Only for the analytical part of test carried out. All other responsibility will be of referring Laboratory.

Approved On : Page 2 of 2

Dr. Krutarth Shah

M.D.  
Microbiologist

Dr. Sandip Shah

M.D. (Path. & Bact.)  
Consultant Pathologist

M.D. (Path. & Bact.)  
Consultant Pathologist

Supratech Micropath Laboratory & Research Institute Pvt. Ltd.  
"KEDAR" Opposite Krupa Petrol Pump, Near Parimal Garden, Ahmedabad - 380 006 | Phone: +91- 79 - 4040 8181 / 6161 8181 / 2640 8181  
Email: contact@supratechlabs.com | CIN : U85195GJ2013PTC077365,2013-14 | Web: www.supratechlabs.com



## LABORATORY REPORT



Case ID : 011151154


Name	:GUARD -AIR (GERMICIDAL UNIT AND RELIABLE DRAWER- AIR PURIFIER) BATCH CODE :112020-A0003 MFG : NOVEMBER 2020(BA-2 : 2 MIN.)	Sex/Age	: Unkown/	Pt ID	:
Ref By	:	Dis.Loc.	:	Pt. Loc.	:
Bill. Loc.	:Supratech billing	Sample Type	: Plate	Ph #	:
Registration Date & Time	: 25-Nov-2020 20:36	Sample Coll. By	:	Ref Id	:
Sample Date & Time	:	Acc. Remarks	:	Ref Id 2	:
Report Date & Time	: 01-Dec-2020 22:03				

### CORONA DISINFECTION INSTRUMENT SURVEILLANCE

GUARD-Air (Germicidal Unit And Reliable Drawer – Air Purifier)

Batch Code: 112020-A0003

MFG: November 2020

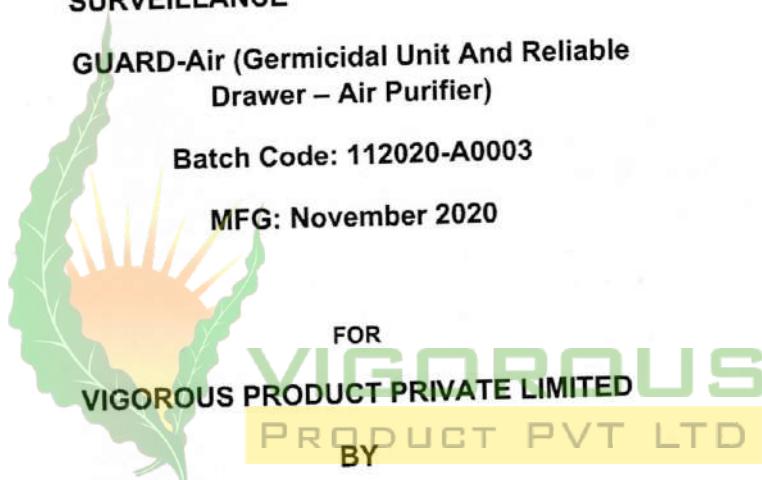

SUPRATECH MICROPATH LABORATORY & RESEARCH INSTITUTE PVT. LTD.

Standard Organism Exposed	Vigorous Antimicrobial Light Exposure Timing	Observation	Result
Bacillus subtilis (ATCC 6051)	2 Minutes	No growth after 02 Minutes	Satisfactory

# For test performed on specimens received or collected from non-STMPL locations, it is presumed that the specimen belongs to the patient named or identified as labeled on the container/test request and such verification has been carried out at the point generation of the said specimen by the sender. STMPL will be responsible Only for the analytical part of test carried out. All other responsibility will be of referring Laboratory.

Approved On : Page 1 of 2

Dr. Krutarth Shah

M.D.

Microbiologist

Dr. Sandip Shah

M.D. (Path. & Bact.)  
Consultant Pathologist

M.D. (Path. & Bact.)  
Consultant Pathologist



Supratech Micropath Laboratory & Research Institute Pvt. Ltd.

"KEDAR" Mapusa House, Petrol Pump, Near Parimal Garden, Ahmedabad - 380 006 | Phone: +91- 79 - 4040 8181 / 6161 8181 / 2640 8181

Email: contact@supratechlabs.com | CIN : U85195GJ2013PTC077365,2013-14 | Web: www.supratechlabs.com

## LABORATORY REPORT



Case ID : 011151154

Name	:GUARD -AIR (GERMICIDAL UNIT AND RELIABLE DRAWER- AIR PURIFIER) BATCH CODE :112020- A0003 MFG : NOVEMBER 2020(BA-2 : 2 MIN.)	Sex/Age	: Unkown/	Pt ID	:
Ref By	:	Dis.Loc.	:	Pt. Loc.	:
Bill. Loc.	:Supratech billing			Ph #	:
Registration Date & Time	: 25-Nov-2020 20:36	Sample Type	: Plate	Ref Id	:
Sample Date & Time	:	Sample Coll. By	:	Ref Id 2	:
Report Date & Time	: 01-Dec-2020 22:03	Acc. Remarks	:		

**Method:** Standard ATCC strain of E.coli (Live culture) was exposed to Vigorous Antimicrobial Light for defined time period. Liquid culture of sample was done thereafter to check for presence of any bacteria.

**Result:** Clearing of Organisms after 02 Minutes of Exposure to Vigorous Antimicrobial Light. (Satisfactory)



----- End Of Report -----

# For test performed on specimens received or collected from non-STMPL locations, it is presumed that the specimen belongs to the patient named or identified as labeled on the container/test request and such verification has been carried out at the point generation of the said specimen by the sender. STMPL will be responsible Only for the analytical part of test carried out. All other responsibility will be of referring Laboratory.

Approved On : Page 2 of 2

Dr. Krutarth Shah

M.D.

Microbiologist

Dr. Sandip Shah

M.D. (Path. & Bact.)

Consultant Pathologist

M.D. (Path. & Bact.)

Consultant Pathologist



COLLEGE OF AMERICAN PATHOLOGISTS

Supratech Micropath Laboratory & Research Institute Pvt. Ltd.

"KEDAR" Opposite Kripa Petrol Pump, Near Parimal Garden, Ahmedabad - 380 006 | Phone: +91- 79 - 4040 8181 / 6161 8181 / 2640 8181

Email: contact@supratechlabs.com | CIN : U85195GJ2013PTC077365,2013-14 | Web: www.supratechlabs.com

## LABORATORY REPORT



Case ID : 011151149


Name	:GUARD -AIR (GERMICIDAL UNIT AND RELIABLE DRAWER- AIR PURIFIER)	Sex/Age	: Unkown/	Dis.Loc.	:	Pt ID	:
Ref By	:DR KKS SIR MICRO					Pt. Loc.	:
Bill. Loc.	:Supratech billing					Ph #	:
Registration Date & Time	: 25-Nov-2020 20:31	Sample Type	: Plate			Ref Id	:
Sample Date & Time	:	Sample Coll. By	:			Ref Id 2	:
Report Date & Time	: 01-Dec-2020 22:01	Acc. Remarks	:				

## CORONA DISINFECTION INSTRUMENT SURVEILLANCE

**GUARD-Air (Germicidal Unit And Reliable Drawer – Air Purifier)**

Batch Code: 112020-A0003

MFG: November 2020

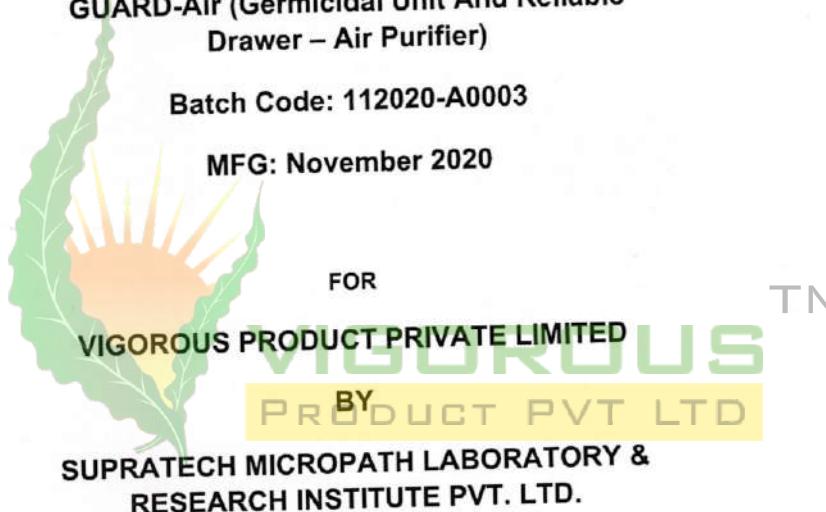

Standard Organism Exposed	Vigorous Antimicrobial Light Exposure Timing	Observation	Result
Escherichia coli (ATCC 25922)	2 Minutes	No growth after 02 Minutes	Satisfactory

# For test performed on specimens received or collected from non-STMPL locations, it is presumed that the specimen belongs to the patient named or identified as labeled on the container/test request and such verification has been carried out at the point generation of the said specimen by the sender. STMPL will be responsible Only for the analytical part of test carried out. All other responsibility will be of referring Laboratory.

Approved On : Page 1 of 2

Dr. Krutarth Shah

M.D.

"KEDAR" Chiropractor

Dr. Sandip Shah

M.D. (Path. & Bact.)  
Consultant Pathologist

M.D. (Path. & Bact.)  
Consultant Pathologist

Supratech Micropath Laboratory & Research Institute Pvt. Ltd.

CAP  
ACCREDITED  
COLLEGE of AMERICAN PATHOLOGISTS

## LABORATORY REPORT



Case ID : 011151149

Name	:GUARD -AIR (GERMICIDAL UNIT AND RELIABLE DRAWER- AIR PURIFIER)	Sex/Age	: Unkown/	Pt ID	:
	BATCH CODE:112020-A0003 MFG			Pt. Loc.	:
	:NOVEMBER 2020 (EC-2 : 2 MIN)			Ph #	:
Ref By	:DR KKS SIR MICRO	Dis.Loc.	:	Ref Id	:
Bill. Loc.	:Supratech billing			Ref Id 2	:
Registration Date & Time	: 25-Nov-2020 20:31	Sample Type	: Plate		
Sample Date & Time	:	Sample Coll. By	:		
Report Date & Time	: 01-Dec-2020 22:01	Acc. Remarks	:		

**Method:** Standard ATCC strain of E.coli (Live culture) was exposed to Vigorous Antimicrobial Light for defined time period. Liquid culture of sample was done thereafter to check for presence of any bacteria.

**Result:** Clearing of Organisms after 02 Minutes of Exposure to Vigorous Antimicrobial Light.  
(Satisfactory)



TM

**VIGOROUS**  
PRODUCT PVT LTD

----- End Of Report -----

# For test performed on specimens received or collected from non-STMPL locations, it is presumed that the specimen belongs to the patient named or identified as labeled on the container/test request and such verification has been carried out at the point generation of the said specimen by the sender.  
STMPL will be responsible Only for the analytical part of test carried out. All other responsibility will be of referring Laboratory.

Approved On : Page 2 of 2

Dr. Krutarth Shah

M.D.

Opposite Kedarkant Patel Pump,

"KEDAR" Opposite Kedarkant Patel Pump,

Dr. Sandip Shah

M.D. (Path. & Bact.)

Consultant Pathologist

Supratech Micropath Laboratory & Research Institute Pvt. Ltd.

M.D. (Path. & Bact.)

Consultant Pathologist



COLLEGE OF AMERICAN PATHOLOGISTS